

## Case Report

**Surgical removal of knotted intravascular device in the right femoral artery Case Report and Review of the Literature****Alejandro Rojas-Marroquín<sup>1,2\*</sup>, Carlos Espinosa<sup>3,4</sup>, Ricardo Ramírez<sup>5,6</sup>, Jharol Jair Rojas<sup>7</sup>**<sup>1</sup>Department of Neurosurgery, Division of Endovascular Neurosurgery, Medilaser Clinic, Tunja, Colombia<sup>2</sup>Endovascular Neurosurgeon, Universidad Nacional Autónoma de México, México DF, México<sup>3</sup>Department of angiology and vascular surgery, Medilaser Clinic, Tunja, Colombia.<sup>4</sup>Angiologist and vascular surgeon, Universidad Militar, Bogotá, Colombia.<sup>5</sup>Department of Anesthesiology, Medilaser Clinic, Tunja, Colombia<sup>6</sup>Anesthesiologist, Universidad Militar, Bogotá, Colombia<sup>7</sup>Male Nurse, UDCA, Bogotá, Colombia**\*Corresponding author**

Alejandro rojas Marroquín

Email: alejorojasm@gmail.com

**Abstract:** We report the case of a 75-year-old female patient who underwent digital subtraction angiography because there was suspicion of cerebral arteriovenous malformation. Fluoroscopy reveals that the Impulse Flextrusion™ Shaft FR4 6F catheter (Boston Scientific) was completely knotted and entrapped in the right femoral artery. We attempted to remove the catheter through the EN Snare Endovascular Snare System, this being unsuccessful, so we decided the surgical exploration of the right femoral artery could completely withdraw the catheter knotted and entrapped without any complication.

**Keywords:** catheters, intravascular devices, knotting, surgical removal.

**INTRODUCTION**

The first knot was described by Johansson et al and published in 1954 [1]. During these more than 60 years, more than a hundred cases have been reported and we have seen the incredible evolution of the endovascular techniques of withdrawal of intravascular devices, which remain the best and most frequent treatment option. However, entrapped and knotted catheters may need to be surgically removed when the knot is large and has many loops [2-4]. Nearly 2/3 of the cases of knotted catheters reported in the literature were successfully removed through endovascular approaches [5]. 1/3 of this population required a surgical approach, with venotomy being the most usual procedure (subclavian vein, jugular vein, femoral vein, basilic vein and saphenous vein) followed by Arteriotomy (femoral artery, axillary artery and carotid artery) and in 5 cases an open cardiomy was required [6, 7]. In this report, we present a case of right femoral arteriotomy for removal of an intravascular device.

**CASE REPORT**

We report the case of a 75-year-old female patient who underwent digital subtraction angiography

because there was suspicion of cerebral arteriovenous malformation. The patient had a previous history of controlled hypertension and dyslipidemia. The procedure was performed through the right femoral artery track using a 7F introducer (Glidesheath™ Terumo Medical Introducer) with an Impulse Flextrusion™ Shaft FR4 6F (Boston Scientific) catheter (Figure 1A and 1B).

Catheter manipulation proved to be very challenging as the patient presented severe tortuosity of the right femoral artery and right iliac artery, requiring the use of a long hydrophilic guidewire. However, we were unable to advance beyond the aortic arch cause to lack of catheter torque. After a prolonged manipulation of the catheter we noticed that it was very difficult to mobilize through it, considering that the fluoroscopy reveals, that the Impulse Flextrusion™ Shaft FR4 6F (Boston Scientific) catheter was completely knotted and entrapped in the right femoral artery (Figure 2A and 2B).



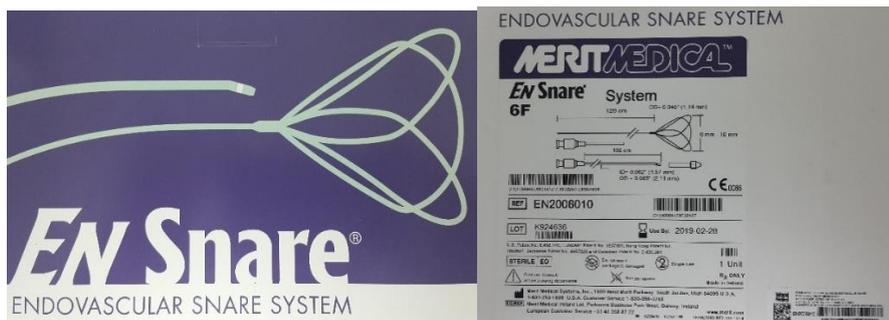


Fig 3A and 3B: EN Snare Endovascular Snare System

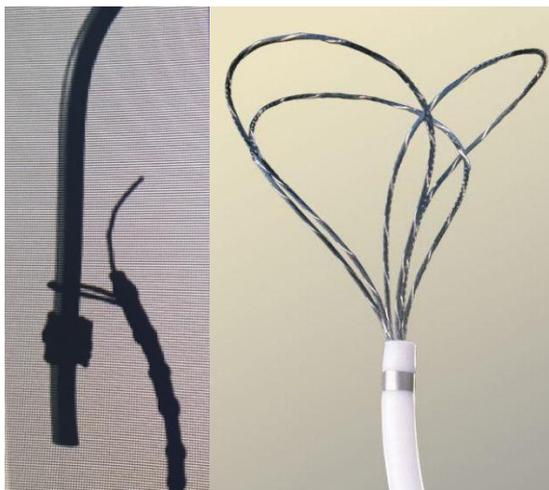


Fig 4A and 4B: EN Snare: It is designed with three interlaced loops to retrieve and manipulate objects.



Fig 5A: Arteriotomy Figure 5B: Right femoral artery suture. (Surgical removal of knotted intravascular device in the right femoral artery)

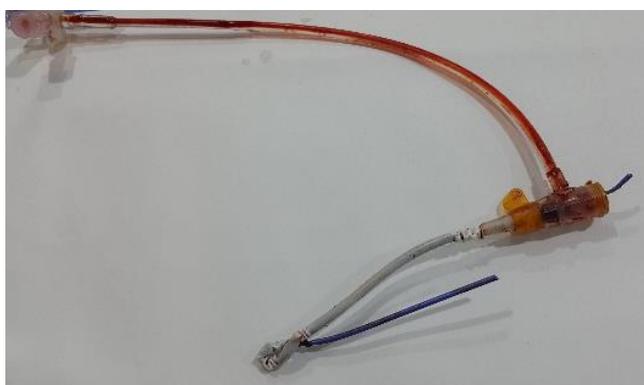


Fig 6: Catheter knotted and entrapped



**Fig 7: Surgical wound closure in right inguinal region**

## DISCUSSION

The surgical approach is an excellent alternative to the usual withdrawal of intravascular devices using interventional radiology techniques. There are many limitations such as the position and severity of the foreign body's knotting that prevent its removal by endovascular techniques, so the surgical option should always be considered.

## CONCLUSIONS

Removal of knotted intravascular devices may be difficult because of, on certain occasions, morphological limitations including blood vessel direction, tortuosity, knot severity, and number of turns in the catheter. Despite great advances in endovascular techniques and devices, it is sometimes necessary to resort to a surgical approach that is an excellent non-complication-free option.

## REFERENCES

1. Hood S, McAlpine HM, Davidson JA. Successful retrieval of a knotted pulmonary artery catheter trapped in the right ventricle using a dormier basket. *Scottish medical journal*. 1997 Dec 1; 42(6):184-.
2. Karanikas ID, Polychronidis A, Vrachatis A, Arvanitis DP, Simopoulos CE, Lazarides MK. Removal of knotted intravascular devices. Case report and review of the literature. *European journal of vascular and endovascular surgery*. 2002 Mar 31; 23(3):189-94.
3. Perreas KG, Kumar S, Khan Z, Rees A. A knot in the heart-surgical removal of a pulmonary artery catheter entangled in the tricuspid valve chordae. *European journal of cardio-thoracic surgery: official journal of the European Association for Cardio-thoracic Surgery*. 1999 Jan; 15(1):112-3.
4. Tan C, Bristow PJ, Segal P, Bell RJ. A technique to remove knotted pulmonary artery catheters.

*Anaesthesia and intensive care*. 1997 Apr; 25(2):160-2.

5. Mehta N, Lochab SS, Tempe DK, Trehan V, Nigam M. Successful nonsurgical removal of a knotted and entrapped pulmonary artery catheter. *Catheterization and cardiovascular diagnosis*. 1998 Jan 1; 43(1):87-9.
6. Abreu AR, Campos MA, Krieger BP. Pulmonary artery rupture induced by a pulmonary artery catheter: a case report and review of the literature. *Journal of Intensive Care Medicine*. 2004 Sep 1; 19(5):291-6.
7. Georghiou GP, Vidne BA, Raanani E. Knotting of a pulmonary artery catheter in the superior vena cava: surgical removal and a word of caution. *Heart*. 2004 May 1; 90(5):e28.